



GSI Equine IL-1 β ELISA Kit- Plasma/Serum DataSheet

Interleukin-1 beta (IL-1 β) also known as catabolin, is a member of the interleukin 1 cytokine family. IL-1 β precursor is cleaved by caspase 1 (interleukin 1 beta convertase). Cytosolic thiol protease cleaves the product to form mature IL-1 β . Interleukin-1 alpha and interleukin-1 beta forms IL-1 (1,2,3).

IL-1 β is produced by activated macrophages as a proprotein, which is proteolytically processed to its active form by caspase 1 (CASP1/ICE). This cytokine is an important mediator of the inflammatory response, and is involved in a variety of cellular activities, including cell proliferation, differentiation, and apoptosis. The induction of cyclooxygenase-2 (PTGS2/COX2) by this cytokine in the central nervous system (CNS) is found to contribute to inflammatory pain hypersensitivity. IL-1 β gene and eight other interleukin 1 family genes form a cytokine gene cluster on chromosome 2(4).

References

1. Auron PE, et al (1984). Proc Natl Acad Sci U S A 81 (24): 7907–11.
2. March CJ, et al. (1985). Nature 315 (6021): 641–7.
3. Clark BD, et al (1986). Nucleic Acids Res 14 (20): 7897–1914.
4. Entrez Gene: IL1B interleukin 1, beta.
<http://www.ncbi.nlm.nih.gov/sites/entrez?Db=gene&Cmd=ShowDetailView&TermToSearch=3553>.

PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique and uses biotin-streptavidin chemistry to improve the performance of the assays. An antibody specific for equine IL-1 β has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any IL-1 β present is bound by the immobilized antibody. After washing away any unbound substances, a detection antibody specific for equine IL-1 β is added to the wells. Following wash to remove any unbound antibody reagent, a detection reagent is added. After intensive wash a substrate solution is added to the wells and color develops in proportion to the amount of IL-1 β bound in the initial step. The color development is stopped and the intensity of the color is measured.

This package insert must be read in its entirety before using this product.

Storage

Store the standard and detection antibody at 4°C ~ -20°C, store 10 x reagent diluents and the antibody pre-coated plate at -20°C and store the rest of the kit at 4°C. The kit can be used in 3 months.



GSI Equine IL-1 β ELISA Kit- Plasma/Serum DataSheet

MATERIALS PROVIDED

| Description | Quantity | Description | Quantity | Description | Quantity |
|--------------------------|----------|----------------------|----------|---------------------|----------|
| Antibody Precoated Plate | 1 | 20 x PBS | 1 | Substrate Solution | 1 |
| Detection Antibody | 1 | 20 x Wash Buffer | 1 | Stop Solution | 1 |
| Detection Agent | 1 | 10 x Reagent Diluent | 1 | DataSheet/Manual | 1 |
| Standard | 3 | Standard Diluent | 1 | 96-well plate sheet | 1 |

Bring all reagents to room temperature before use.

1 x **96-well Plate precoated with equine IL-1 β capture antibody**-Store at -20°C upon received.

Equine IL-1 β Detection Antibody– The lyophilized Detection Antibody should be stored at 4°C ~ -20°C in a manual defrost freezer for up to 6 months, if not used immediately. Centrifuge for 1 min at 6000 x g to bring down the material prior to open the vial. The vial contains sufficient Detection Antibody for a 96-well plate. Add 200 μ L 1 x Reagent Diluent to the antibody vial and vortex 20 sec and allow it to sit for 5 min prior to use. Take 200 μ L of detection antibody to 9.8 mL Reagent Diluent if the entire 96-well plate is used. If the partial antibody is used store the rest at -20°C until use.

Equine IL-1 β Standard (3 vials) – The lyophilized Equine IL-1 β Standard has a total of 3 vials. Each vial contains the standard sufficient for a 96-well plate. The un-reconstituted standard can be stored at 4°C ~ -20°C for up to 3 months if not used immediately. Centrifuge for 1 min at 6000 x g to bring down the material prior to open the vial. Add 500 μ L of Standard Diluent to a Standard vial to make the high standard concentration of 6000 pg /ml. Vortex 20 sec and allow it to sit for 5 min prior to use. A seven point standard curve is generated using 2-fold serial dilutions in Standard Diluent, vortex 20 sec for each of dilution step.

Detection Agent (50 μ L) – Centrifuge for 1 min at 6000 x g to bring down the material prior to open the vial. The vial contains sufficient Detection Agent for a 96-well plate. If the volume is less than 50 μ L, add 1 x Reagent Diluent to a final volume of 50 μ L and vortex briefly. Make 1:200 dilution in Reagent Diluent. If the entire 96-well plate is used, add 50 μ L of Detection Agent to 10 mL Reagent Diluent prior to the assay. The rest of undiluted Detection Reagent can be stored at 4°C for up to 6 months. **DO NOT FREEZE.**

20 x PBS, pH 7.3, 30 mL- Dilute to 1 x PBS with deionized distilled water and mix well prior to use.

20 x Wash Buffer, 25 mL- Dilute to 1 x Wash Buffer with 1 x PBS prior to use.

10 x Reagent Diluent, 3 mL –Store at -20 °C. Prior to use dilute to 1 x Reagent Diluent with 1 x PBS.

Standard Diluent, 15 mL.

Substrate Solution, 10 mL.

Stop Solution, 5 mL.



GSI Equine IL-1 β ELISA Kit- Plasma/Serum DataSheet

Assay Procedure

1. Lift the plate cover at the top left corner and cover the wells that are not used. Vortex briefly the samples prior to the assay. Add 100 μ L of plasma or serum or less to each well, and in each well add PBS to a total volume of 100 μ L if the sample is less than 100 μ L. Add 100 μ L of standards per well and use duplicate wells for each standard or sample. Cover the 96-well plate and incubate 2 hour at room temperature.
2. Aspirate each well and wash with 1 x Wash Buffer, repeating the process two times for a total of three washes. Wash by filling each well with 1 x Wash Buffer (300 μ L) using a multi-channel pipette, manifold dispenser or auto-washer. Complete removal of liquid at each step is essential for good performance. After the last wash, remove any remaining Wash Buffer by aspirating or by inverting the plate and blotting it against clean paper towels.
3. Add 100 μ L of the working dilution of the Detection Antibody to each well. Cover the plate and incubate 2 hour at room temperature.
4. Repeat the aspiration/wash as in step 2.
5. Add 100 μ L of the working dilution of Detection Agent to each well. Cover the plate and incubate for 20 minutes at room temperature. Avoid placing the plate in direct light.
6. Repeat the aspiration/wash as in step 2.
7. Add 100 μ L of Substrate Solution to each well. Incubate for 10 minutes at room temperature. Avoid placing the plate in direct light.
8. Add 50 μ L of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
9. Determine the optical density of each well immediately, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

Precaution and Technical Notes

1. Thorough mixing of the standard at each step of the dilutions is critical to ensure a normal calibration curve. A standard curve should be generated for each set of samples assayed.
2. If IL-1 β exceeds the upper limit of the detection, the sample needs to be diluted with PBS. The dilution factor must be used for calculation of the concentration.
3. Detection Agent contains enzyme, DO NOT mass up with Detection Antibody.
4. The Stop Solution is an acid solution, handle with caution.
5. This kit should not be used beyond the expiration date on the label.
6. A thorough and consistent wash technique is essential for proper assay performance. Wash Buffer should be dispensed forcefully and removed completely from the wells by aspiration or decanting. Remove any remaining Wash Buffer by aspiration or by inverting the plate and blotting it against clean paper towels.
7. Use a fresh reagent reservoir and pipette tips for each step.
8. It is recommended that all standards and samples be assayed in duplicate.
9. Avoid microbial contamination of reagents and buffers. This may interfere with the sensitivity of the assay.

GSI Equine IL-1 β ELISA Kit- Plasma/Serum DataSheet


Calculation of Results

Average the duplicate readings for each standard, control, and sample and subtract the average zero (blank) standard optical density.

Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the IL-1 β concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

The Standard Curve

The graph below represents typical data generated when using this equine IL-1 β ELISA Kit. The standard curve was calculated using a computer generated 4-PL curve-fit. For this case, a Bio-Rad iMark™ Microplate Reader and a Microplate Manager 6 Software were used to generate this curve. The correlation coefficient (r^2) is 0.998-1.000.

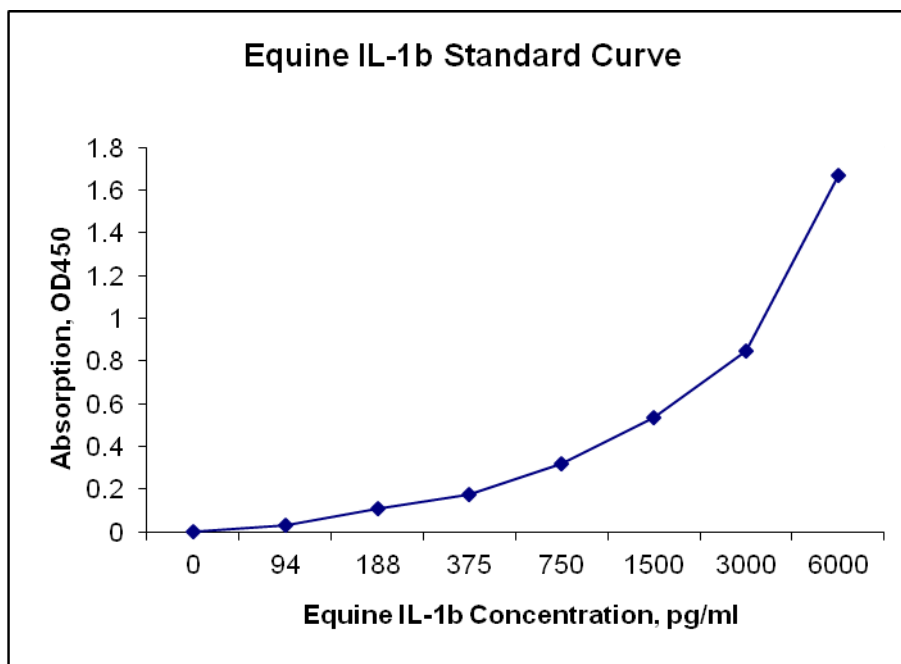



GSI Equine IL-1 β ELISA Kit- Plasma/Serum DataSheet

Specificity

The following recombinant equine proteins prepared at 1 ng/ml were tested and exhibited no cross-reactivity or interference.

BMP1, BMP2, BMP4, IL-2, IL-4, IL-5, IL-6, IL-8, IL-10, IL-15, IFN γ , TGF β 1, TGF β 2, TGF β 3, TLR2, TNF- α .

Calibration

This kit is calibrated against a highly purified yeast-expressed recombinant equine IL-1 β .

Detection Range

1-6000 pg/ml

Assay Sensitivity

0.6 pg/ml

Assay Precision

Intra-Assay %CV: 6; Inter-Assay %CV: 11

For Research Use Only

Related products

20 x Sample Diluent, GERC-103058

20 x PBS, Cat. 103004-20

10 x ELISA Wash Buffer, Cat. 103028

10 x ELISA Reagent Diluent, Cat. GERC-103055

Universal Blocking Buffer, Cat.103005

2 x Recombinant Protein Stabilizer, Cat. GERC-03014-2

5 x Recombinant Protein Stabilizer, Cat. GERC-103014-5

ELISA G-Blue Substrate Solution, Cat. 103021

Equine IL-1 β Standard

Equine IL-1 β Detection Antibody

Detection Agent