



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet

14-3-3 proteins are a family of conserved regulatory molecules that are expressed in all eukaryotic cells. 14-3-3 proteins have the ability to bind a multitude of functionally diverse signaling proteins, including kinases, phosphatases, and transmembrane receptors. More than 200 signaling proteins have been reported as 14-3-3 ligands. The 14-3-3 proteins eluted in the 14th fraction of Rabbit brain homogenate and were found on positions 3.3 of subsequent electrophoresis by Moore and Perez (1967). Elevated amounts of 14-3-3 proteins are found in the cerebrospinal fluid of patients with Creutzfeldt-Jakob disease.^[1] There are seven genes that encode seven distinct 14-3-3 proteins in most mammals. Eukaryotes can tolerate the loss of a single 14-3-3 gene if multiple genes are expressed, however deletion of all 14-3-3s (as experimentally determined in yeast) results in death. 14-3-3 proteins can be considered evolved members of the Tetrapeptide Repeat (TPR) superfamily, generally have 9 or 10 alpha helices, and usually form homo- and/or hetero-dimer interactions along their amino-terminal helices. These proteins contain a number of known common modification domains, including regions for divalent cation interaction, phosphorylation^[2] & acetylation, and proteolytic cleavage, among others established and predicted. 14-3-3 proteins play an isoform-specific role in class switch recombination. They are believed to interact with the protein Activation-Induced (Cytidine) Deaminase in mediating class switch recombination. Phosphorylation of Cdc25C by CDS1 and CHK1 creates a binding site for the 14-3-3 family of phosphoserine binding proteins. Binding of 14-3-3 has little effect on Cdc25C activity, and it is believed that 14-3-3 regulates Cdc25C by sequestering it to the cytoplasm, thereby preventing the interactions with CycB-Cdk1 that are localized to the nucleus at the G2/M transition.^[3]

References

1. Takahashi H et al. (1999). *Clinical and Diagnostic Laboratory Immunology* **6** (6): 983–5.
2. Madhurima S et al. (2012). *Biochemical Journal*. doi:10.1042/BJ20120938.
3. Jahn TP et al. (2002). *The Journal of Biological Chemistry* **277** (8): 6353–6358.

PRINCIPLE OF THE ASSAY

This ELISA kit is for quantification of 14-3-3 eta in Rabbit. This is a quick ELISA assay that reduces time to 50% compared to the conventional method, and the entire assay only takes 3 hours. This assay employs the quantitative sandwich enzyme immunoassay technique and uses biotin-streptavidin chemistry to improve the performance of the assays. An antibody specific for Rabbit 14-3-3 eta has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any 14-3-3 eta present is bound by the immobilized antibody. After washing away any unbound substances, a detection antibody specific for Rabbit 14-3-3 eta is added to the wells. Following wash to remove any unbound antibody reagent, a detection reagent is added. After intensive wash a substrate solution is added to the wells and color develops in proportion to the amount of 14-3-3 eta bound in the initial step. The color development is stopped and the intensity of the color is measured.

This package insert must be read in its entirety before using this product.

Storage

Store at 4 °C. The kit should be used in 3 months.



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet

MATERIALS PROVIDED

Description	Quantity	Description	Quantity	Description	Quantity
Antibody Precoated Plate	2	20 x PBS	2	Substrate Solution	1
Detection Antibody	2	80 x Assay Buffer	1	Stop Solution	1
Conjugate	1	2 x Reagent Diluent	1	DataSheet	1
Standard	4	MSDS/CoA	1	96-well plate sheet	2

Bring all reagents to room temperature before use.

Reagent Preparations

Rabbit 14-3-3 eta Detection Antibody (2 vials) – The lyophilized Detection Antibody should be stored at 4°C for up to 3 months, if not used immediately. Centrifuge for 1 min at 6000 x g to bring down the material prior to open the vial. Each vial contains sufficient Detection Antibody for a 96-well plate. Add 200 µL of sterile 1 x PBS and vortex 30 sec. If the entire 96-well plate is used, take 200 µL of detection antibody to 10.5 mL of 1 x Reagent Diluent to make **Working dilution of detection antibody** and mix thoroughly prior to the assay. If the partial antibody is used store the rest at -20°C until use.

Rabbit 14-3-3 eta Standard (4 vials) – The lyophilized Rabbit 14-3-3 eta Standard has a total of 4 vials. Each vial contains the standard sufficient for generating a standard curve. The unreconstituted standard can be stored at 4°C for up to 3 months if not used immediately. Centrifuge for 1 min at 6000 x g to bring down the material prior to open the tube. Add 500 µL of 1 x Assay Buffer to make the high standard concentration of 4000 pg/ml and vortex for 30 sec. A seven-point standard curve is generated using 2-fold serial dilutions in the Assay Buffer, vortex 30 sec for each of dilution step.

Conjugate (106 µl) – Centrifuge for 1 min at 6000 x g to bring down the material prior to open the vial. The vial contains 106 µL Conjugate sufficient for two 96-well plates. If the volume is less than 106 µL, add sterile 1 x PBS to reach 106 µL and vortex 10 sec. Make 1:200 dilutions in 1 x Reagent Diluent. If the entire 96-well plate is used, add 53 µL of Conjugate to 10.5 mL of 1 x Reagent Diluent to make **working dilution of Conjugate** and mix thoroughly prior to the assay. The rest of undiluted Conjugate can be stored at 4°C for up to 3 months. **DO NOT FREEZE.**

20 x PBS, pH 7.3, 2 x 30 mL- Dilute to 1 x PBS with deionized distilled water and mix well prior to use.

80 x Assay Buffer, 10 mL- Dilute to 1 x Assay Buffer with 1 x PBS prior to use.

2 x Reagent Diluent, 21 mL- Dilute to 1 x Reagent Diluent with 1 x PBS prior to use.

Substrate Solution, 21 mL.

Stop Solution, 11 mL.



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet

Assay Procedure

1. Lift the plate cover and cover the wells that are not used using the strip provided. Vortex briefly the samples prior to the assay. Add 100 μ L of **sample** (such as plasma or serum) or **standard** per well and use duplicate wells for each standard or sample. Cover the 96-well plate and incubate 1 hour at room temperature.
2. Aspirate each well and wash with **1 x Assay Buffer**, repeating the process two times for a total of three washes. Wash by filling each well with 1 x Assay Buffer (300 μ L) using a multi-channel pipette, manifold dispenser or auto-washer. Complete removal of liquid at each step is essential for good performance. After the last wash, remove any remaining Assay Buffer by aspirating or by inverting the plate and blotting it against clean paper towels.
3. Add 100 μ L of the **working dilution of Detection Antibody** to each well. Cover the plate and incubate 1 hour at room temperature.
4. Repeat the aspiration/wash as in step 2.
5. Add 100 μ L of **the working dilution of Conjugate** to each well. Cover the plate and incubate for 20 minutes at room temperature. Avoid placing the plate in direct light.
6. Repeat the aspiration/wash as in step 2.
7. Add 100 μ L of **Substrate Solution** to each well. Incubate for 10-20 minutes at room temperature. Avoid placing the plate in direct light.
8. Add 50 μ L of **Stop Solution** to each well. Gently tap the plate to ensure thorough mixing.
9. Determine the optical density of each well immediately, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

Precaution and Technical Notes

1. It is critical to follow the procedure step by step otherwise appropriate color development may not occur as expected.
2. A standard curve should be generated for each set of samples assayed. Thorough mixing of the standards at each step of the dilutions is critical to ensure a normal standard curve.
3. Plasma or serum sample should be diluted with equal volume of 1 x Assay Buffer and vortex for 1 min prior to assay. If the OD value still exceeds the upper limit of the standard curve, further dilution is recommended till it falls in the detection range and the dilution factor must be used for calculation of the concentration.
4. Conjugate contains enzyme, DO NOT mass up with Detection Antibody.
5. The Stop Solution is an acid solution, handle with caution.
6. This kit should not be used beyond the expiration date on the label.
7. A thorough and consistent wash technique is essential for proper assay performance.
8. Use a fresh reagent reservoir and pipette tips for each step.
9. It is recommended that all standards and samples be assayed in duplicate.
10. Avoid microbial contamination of reagents and buffers. This may interfere with the sensitivity of the assay.



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet


Calculation of Results

Average the duplicate readings for each standard, control, and sample and subtract the average zero (blank) standard optical density.

Create a standard curve by reducing the data using computer software capable of generating a four-parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the 14-3-3 eta concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

The Standard Curve

The graph below represents typical data generated when using this Rabbit 14-3-3 eta ELISA Kit. The standard curve was calculated using a computer generated 4-PL curve-fit. For this case, a Bio-Rad iMark™ Microplate Reader and a Microplate Manager 6 Software were used to generate this curve. The correlation coefficient (r^2) is 0.999-1.000.

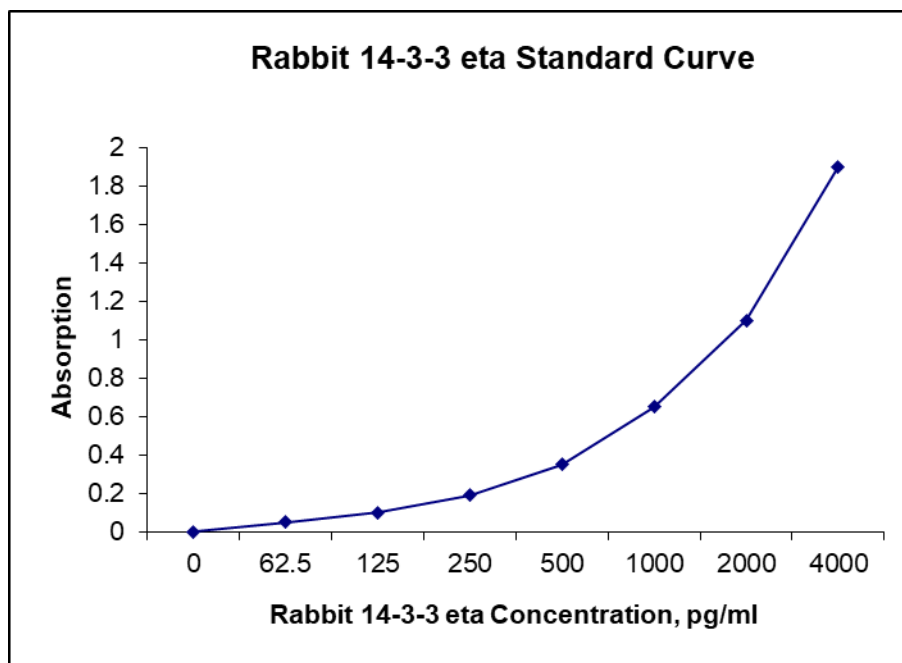



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet

Specificity

The following recombinant Rabbit proteins prepared at 1 ng/ml were tested and exhibited no cross-reactivity or interference.

Adiponectin, ApoAI, BMP1, BMP2, BMP3, BMP4, BMP5, BMP6, BMP7, CCL2, CCL4, CCL5, CRP, FGF acidic, HGF, HSP27, IGF-1, IL-1 α , IL-1 β , IL-1ra, IL-4, IL-5, IL-6, IL-8, IL-10, IL-12, IL-13, IL-15, IL-17C, 14-3-3 ETA1, 14-3-3 ETA3, IFN- α , IFN- β , IFN γ , MMP-2, MMP-3, MMP-9, PDGF, PLA2G7, prolactin, TLR1, TLR2, TLR3, TLR4, TLR9, TGF- β 1, TGF- β 2, TGF- β 3, TNF- α , TNF RI, TNF RII, VEGF, VEGF-R1.

Calibration

This kit is calibrated against a highly-purified yeast-expressed recombinant Rabbit 14-3-3 eta.

Detection Range

62-4,000 pg/ml

Assay Sensitivity

12 pg/ml

Assay Precision

Intra-Assay %CV: 5; Inter-Assay %CV: 10

For Research Use Only

Related products

20 x sample diluent, GR103061
10 x ELISA Assay Buffer, GR103014
10 x Reagent Diluent, GR103028
20 x PBS, GR103004-20
ELISA Substrate, GR103021
ELISA Stop Solution, GR103055
ELISA Conjugate, GR103044
Rabbit 14-3-3 eta standard
Rabbit 14-3-3 eta detection antibody



Nori® Rabbit 14-3-3 eta ELISA Kit -2 Plates DataSheet

Troubleshooting Guide

Problem	Possible causes	Solution
Poor standard curve	<ul style="list-style-type: none">• Inaccurate pipetting• Improper standard curve	<ul style="list-style-type: none">• Check pipettes• Check and use the correct dilution buffer• Vortex 30 sec for each of standard dilution steps
Low signal	<ul style="list-style-type: none">• Improper preparation of standard, samples, detection antibody, and/or conjugate• Too brief incubation times• Inadequate reagent volume or improper dilution	<ul style="list-style-type: none">• Briefly spin down vials before opening. Reconstitute the powder thoroughly.• Ensure sufficient incubation time.• Check pipettes and ensure correct preparation.
Large CV	<ul style="list-style-type: none">• Inaccurate pipetting and mixing• Improper standard/sample dilutions.• Air bubbles in wells.	<ul style="list-style-type: none">• Check pipettes and ensure thorough mixing.• Use the correct dilution buffers• Remove bubbles in wells.
High background	<ul style="list-style-type: none">• Plate is insufficiently washed.• Contaminated Assay Buffer	<ul style="list-style-type: none">• Review the datasheet for proper wash. If using a plate washer, ensure that all ports are unobstructed.• Make fresh Assay Buffer
No signal detected	<ul style="list-style-type: none">• The procedure was misconducted.	<ul style="list-style-type: none">• Ensure the step-by-step protocol was correctly followed and no misstep was conducted.
Low sensitivity	<ul style="list-style-type: none">• Improper storage of the ELISA kit• Stop solution	<ul style="list-style-type: none">• Store standards and detection antibody at -20°C after reconstitution, others at 4°C. Keep substrate protected from light.• Adding stop solution to each well before reading plate